




PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION  
International Bureau

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification 7 : <b>G01S 7/52</b>	<b>A1</b>	(11) International Publication Number: <b>WO 00/20885</b> (43) International Publication Date: 13 April 2000 (13.04.00)
(21) International Application Number: PCT/EP99/07474 (22) International Filing Date: 30 September 1999 (30.09.99) (30) Priority Data: 60/102,923                      1 October 1998 (01.10.98)                      US 09/335,059                      17 June 1999 (17.06.99)                      US (71) Applicant: KONINKLIJKE PHILIPS ELECTRONICS N.V. [NL/NL]; Groenewoudseweg 1, NL-5621 BA Eindhoven (NL). (72) Inventors: JAGO, James, R.; Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL). ENTREKIN, Robert, R.; Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL). (74) Agent: SCHOUTEN, Marcus, M.; Internationaal Octrooibureau B.V., Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL).		(81) Designated States: JP, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).  Published With international search report.
(54) Title: ULTRASONIC DIAGNOSTIC IMAGING SYSTEM WITH BLURRING-CORRECTED SPATIAL COMPOUNDING		

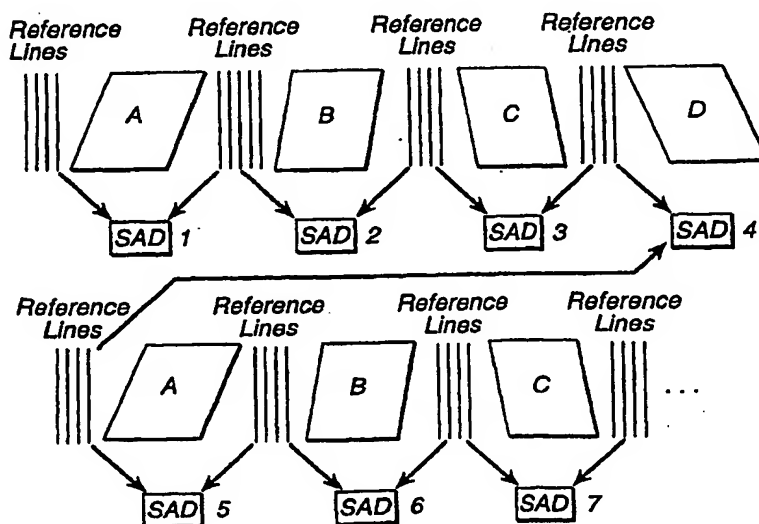

## Abstract

An ultrasonic diagnostic imaging system is described in which the component ultrasonic images which are to be spatially compounded are first registered for misregistration prior to compounding. The component images may be registered to a reference image or registered to form intermediate compound images which are then registered and compounded. The misregistration may be sensed by calculating a similarity metric for a region of interest of the image frames being registered, or on the basis of reference lines acquired for the purpose of registering images.

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon	KR	Republic of Korea	PL	Poland		
CN	China	KZ	Kazakhstan	PT	Portugal		
CU	Cuba	LC	Saint Lucia	RO	Romania		
CZ	Czech Republic	LI	Liechtenstein	RU	Russian Federation		
DE	Germany	LK	Sri Lanka	SD	Sudan		
DK	Denmark	LR	Liberia	SE	Sweden		
EE	Estonia			SG	Singapore		

## Ultrasonic diagnostic imaging system with blurring-corrected spatial compounding.

This application claims the benefit of Provisional U.S. Patent Application serial number 60/102,923, filed October 1, 1998. This application is being concurrently filed with U.S. Application serial number [ATL-196], entitled "Method for correcting blurring of spatially compounded ultrasonic diagnostic images."

5           This invention relates to ultrasonic diagnostic imaging systems and, in particular, to ultrasonic diagnostic imaging systems which produce spatially compounded images which are corrected for image blurring.

Spatial compounding is an imaging technique in which a number of ultrasound images of a given target that have been obtained from multiple vantage points or angles are  
10 combined into a single compounded image by combining the data received from each point in the compound image target which has been received from each angle. Examples of spatial compounding may be found in US Patents 4649927; 4319489; and 4159462. Real time spatial compound imaging is performed by rapidly acquiring a series of partially overlapping component image frames from substantially independent spatial directions, utilizing an array  
15 transducer to implement electronic beam steering and/or electronic translation of the component frames. The component frames are combined into a compound image by summation, averaging, peak detection, or other combinational means. The acquisition sequence and formation of compound images are repeated continuously at a rate limited by the acquisition frame rate, that is, the time required to acquire the full complement of scanlines  
20 over the selected width and depth of imaging.

The compounded image typically shows lower speckle and better specular reflector delineation than conventional ultrasound images from a single viewpoint. Speckle is reduced (i.e. speckle signal to noise ratio is improved) by the square root of N in a compound image with N component frames, provided that the component frames used to create the  
25 compound image are substantially independent and are averaged. Several criteria can be used to determine the degree of independence of the component frames (see, e.g., O'Donnell et al. in IEEE Trans. UFFC v.35, no.4, pp 470-76 (1988)). In practice, for spatial compound imaging with a steered linear array, this implies a minimum steering angle between component frames. This minimum angle is typically on the order of several degrees.

The second way that spatial compound scanning improves image quality is by improving the acquisition of specular interfaces. For example, a curved bone-soft tissue interface produces a strong echo when the ultrasound beam is exactly perpendicular to the interface, and a very weak echo when the beam is only a few degrees off perpendicular. These  
5 interfaces are often curved, and with conventional scanning only a small portion of the interface is visible. Spatial compound scanning acquires views of the interface from many different angles, making the curved interface visible and continuous over a larger field of view. Greater angular diversity generally improves the continuity of specular targets. However, the angular diversity available is limited by the acceptance angle of the transducer  
10 array elements. The acceptance angle depends on the transducer array element pitch, frequency, and construction methods.

The challenges of acquiring images which are in spatial alignment, or of spatially aligning separate images after they have been received, can be considerable. When the objective is to produce spatially compounded images in real time, an even greater  
15 challenge is presented. Image processing must be fast and efficient so that the frame rate of compound images appears to be in real time. The compound images can suffer from motion artifacts, as organs such as the heart and blood vessels can be continually moving as the image data to be compounded is acquired.

One of the problems associated with real time spatial compound imaging is that  
20 several image acquisitions are needed to produce each new compound image frame. The time needed to acquire a spatial compound image consisting of N component frames is approximately N times longer than that of each individual component frame. It is generally desirable to acquire a large number of component frames to maximize the image quality of the compound image. However, since the images to be compounded are acquired temporally, the  
25 compounding of the images can produce a blurred resultant image. Image blurring occurs in real time spatial compound imaging because common features in the acquired component frames do not superimpose exactly when compounded. Misregistration between acquisition frames can occur for a number of reasons, such as:

1. features can shift position within the image plane due to scanhead and/or patient  
30 movement during acquisition (in-plane motion misregistration). This kind of misregistration can be global (translation and/or rotation of entire image) or local (image distortion due to cardiac or respiratory motion, or compression of the tissue with the scanhead).

2. features can shift position due to an incorrect assumption regarding the speed of sound, causing the features to be rendered with axial and angular misregistration (SOS misregistration). This kind of misregistration can be due to an incorrect mean speed of sound or variations in local speed of sound within different tissue types.

5           Accordingly, it is desirable to prevent blurring from causes such as these when compounding images for real time display.

          In accordance with the principles of the present invention, blurring of a compound image is reduced and image quality improved through correction of misregistration errors by registering the component frames to each other prior to compounding. This is  
10   possible by the application of image registration techniques. Image registration is meant here as a general term to describe any process which estimates global and/or local displacement information between two images, and warps one (or both) images to make them congruent with each other. A number of techniques may be used to estimate the displacement, including  
15   cross correlation search, block matching algorithms, maximum brightness, and feature extraction and tracking. Warping algorithms may be first order, global transformations (translation and/or rotation) or higher order (complex local warping), based on the nature and magnitude of the displacements. The component frames are registered to each other prior to compounding, improving image quality.

20

          In the drawings:

          Fig. 1 illustrates in block diagram form an ultrasonic diagnostic imaging system constructed in accordance with the principles of the present invention;

          Fig. 2 illustrates in block diagram form a preferred implementation of the  
25   spatial compounding processor of Fig. 1;

          Fig. 3 illustrates a flowchart for registering all of the constituent frames of a compound image to one reference frame;

          Fig. 4 illustrates a flowchart for pyramid registration of the constituent frames of a compound image;

30           Fig 5 illustrates a flowchart for the successive registration and compounding of the constituent frames of a compound image;

          Fig. 6 illustrates a flowchart for pyramidal registration of non-sequential image frames to form a compound image;

Fig. 7 illustrates a flowchart for the successive registration and compounding of new component frames in conjunction with the removal of old component frames from the compound image; and

Fig. 8 illustrates the use of reference lines for image registration.

- 5 Referring first to Fig. 1, an ultrasonic diagnostic imaging system constructed in accordance with the principles of the present invention is shown. A scanhead 10 including an array transducer 12 transmits beams at different angles over an image field denoted by the dashed rectangle and parallelograms. Three groups of scanlines are indicated in the drawing, labeled A, B, and C with each group being steered at a different angle relative to the scanhead.
- 10 The transmission of the beams is controlled by a transmitter 14 which controls the phasing and time of actuation of each of the elements of the array transducer so as to transmit each beam from a predetermined origin along the array and at a predetermined angle. The echoes returned from along each scanline are received by the elements of the array, digitized as by analog to digital conversion, and coupled to a digital beamformer 16. The digital beamformer delays and
- 15 sums the echoes from the array elements to form a sequence of focused, coherent digital echo samples along each scanline. The transmitter 14 and beamformer 16 are operated under control of a system controller 18, which in turn is responsive to the settings of controls on a user interface 20 operated by the user of the ultrasound system. The system controller controls the transmitter to transmit the desired number of scanline groups at the desired angles, transmit
- 20 energies and frequencies. The system controller also controls the digital beamformer to properly delay and combine the received echo signals for the apertures and image depths used.

- The scanline echo signals are filtered by a programmable digital filter 22, which defines the band of frequencies of interest. When imaging harmonic contrast agents or performing tissue harmonic imaging the passband of the filter 22 is set to pass harmonics of
- 25 the transmit band. The filtered signals are then detected by a detector 24. In a preferred embodiment the filter and detector include multiple filters and detectors so that the received signals may be separated into multiple passbands, individually detected and recombined to reduce image speckle by frequency compounding. For B mode imaging the detector 24 will perform amplitude detection of the echo signal envelope. For Doppler imaging ensembles of
- 30 echoes are assembled for each point in the image and are Doppler processed to estimate the Doppler shift or Doppler power intensity.

In accordance with the principles of the present invention the digital echo signals are processed by spatial compounding in a processor 30. The digital echo signals are initially pre-processed by a preprocessor 32. The pre-processor 32 can preweight the signal

samples if desired with a weighting factor. The samples can be preweighted with a weighting factor that is a function of the number of component frames used to form a particular compound image. The pre-processor can also weight edge lines that are at the edge of one overlapping image so as to smooth the transitions where the number of samples or images which are compounded changes. The pre-processed signal samples may then undergo a resampling in a resampler 34. The resampler 34 can spatially realign the estimates of one component frame or to the pixels of the display space. This may be desirable when there is motion between image frames, there is motion within an image, or there is scanhead motion during image acquisition.

10           After resampling the image frames are compounded by a combiner 36. Combining may comprise summation, averaging, peak detection, or other combinational means. The samples being combined may also be weighted prior to combining in this step of the process. Finally, post-processing is performed by a post-processor 38. The post-processor normalizes the combined values to a display range of values. Post-processing can be most easily implemented by look-up tables and can simultaneously perform compression and mapping of the range of compounded values to a range of values suitable for display of the compounded image.

          The compounding process may be performed in estimate data space or in display pixel space. In a preferred embodiment scan conversion is done following the compounding process by a scan converter 40. The compound images may be stored in a Cineloop® memory 42 in either estimate or display pixel form. If stored in estimate form the images may be scan converted when replayed from the Cineloop memory for display. The scan converter and Cineloop memory may also be used to render three dimensional presentations of the spatially compounded images as described in U.S. Patents 5,485,842 and 5,860,924. Following scan conversion the spatially compounded images are processed for display by a video processor 44 and displayed on an image display 50.

          Fig. 2 illustrates a preferred implementation of the spatial compounding processor 30 of Fig. 1. The processor 30 is preferably implemented by one or more digital signal processors 60 which process the image data in various ways. The digital signal processors 60 can weight the received image data and can resample the image data to spatially align pixels from frame to frame, for instance. The digital signal processors 60 direct the processed image frames to a plurality of frame memories 62 which buffer the individual image frames. The number of image frames capable of being stored by the frame memories 62 is preferably at least equal to the maximum number of image frames to be compounded such as

sixteen frames. In accordance with the principles of the present invention, the digital signal processors are responsive to control parameters including image display depth, depth of region of greatest compounding, clinical application, compound display rate, mode of operation, and acquisition rate for determining the number of images to compound at a given instant in time.

5 The digital signal processors select component frames stored in the frame memories 62 for assembly as a compound image in accumulator memory 64. The compounded image formed in the accumulator memory 64 is weighted or mapped by a normalization circuit 66, then compressed to the desired number of display bits and, if desired, remapped by a lookup table (LUT) 68. The fully processed compounded image is then transmitted to the scan converter for

10 formatting and display.

In accordance with the principles of the present invention, the image data of the component frames used to form a compound image is resampled to spatially register the component frames prior to compounding, thereby improving image quality by reducing blurring effects of overlapping unregistered image data. The resampling and registration of

15 component image frames is performed by the programming of the digital signal processors 60, which operate upon component images stored in the frame memories 62. The final registered and compounded image is then stored in the accumulator memory 64. Prior art techniques have used image registration methods for estimating intrinsic tissue properties, such as speed of sound or elasticity, as diagnostic parameters (e.g., Robinson et. al. in Ult. in Med. & Biol., v.17, no.6, pp 633-46 (1991) and Ophir et al. in Euro. J. Ult., v.3, pp 49-70 (1996)), or for

20 estimating scanhead motion to produce a static "panoramic" image (e.g., U.S. Patent 5,566,674).

There are many possible implementations for image registration prior to compounding in accordance with the present invention. Fig. 3 illustrates one embodiment, the

25 "reference frame" method, as applied to a four frame acquisition sequence. The four constituent frames for compounding are shown as A, B, C, and D in temporal sequence in Fig. 3. One of the component frames (A) is designated as the "reference frame," and as subsequent frames (B,C,D) are acquired, they are warped so that their features are congruent with corresponding features of frame A. As the flowchart shows, when frame B is acquired it is

30 registered with frame A, then frame C is acquired and registered with frame A, then frame D is acquired and registered with frame A. After all four constituent frames have been acquired and registered, the aligned frames are compounded. The process is repeated with each new acquisition sequence (E,F,G,H with E designated as the new reference frame). Alternatively, the reference frame can be updated with each new acquisition frame (B, C, D, E with B as the



reference frame; C,D,E,F with C as the reference frame; etc.) Any one of the frames of each four frame sequence may be designated as the reference frame.

Fig. 4 illustrates a second embodiment in which pairs of images are registered and compounded, followed by a second step of registration and compounding of the previously registered and compounded pairs, termed herein as the "pyramid" method. Fig. 4 illustrates the pyramid technique for four component images A, B, C, and D. In the first step of the method the A and B frames are registered and compounded, then the C and D frames are registered and compounded. These intermediate compounded images, identified as U and V, are then registered and compounded to form the final compound image.

If only partial correction of the misregistration error is acceptable (or if conditions exist where registration of all component frames may be unreliable), then the first registration step can be omitted, gaining a substantial reduction in computational requirements. In that case the temporally adjacent images A and B are compounded, as are temporally adjacent images C and D. The resulting two intermediate compounded images, U and V, are then registered and compounded. Another alternative is to register frames A and B and then frames C and D, compound the registered frame pairs, then omit the last registration step and simply compound the intermediate U and V images to form the final compound image.

Fig. 7 illustrates a further aspect of the present invention which is that, while the A,C,B,D frame sequence in this drawing is temporally sequential, the temporally adjacent frames are not spatially adjacent. That is, the look direction of frame C is not the angularly similar look direction of frame B, but is at a significantly different look direction from that of frame A, the frame with which it is initially compounded. The same is true of the B and D frame pair. This will result in the best possible intermediate compounded images U and V, since the temporal adjacency will reduce motion artifacts while the more greatly divergent look directions will reduce the anisotropy in the compounded image.

Fig. 5 shows yet another embodiment where the compound image is accumulated frame by frame with successive registration and compounding steps. In the illustrated embodiment images A and B are registered and compounded to form a first intermediate compound image B'. Image B' is then registered and compounded with image C to form a further intermediate compound image C'. Image C' is then registered and compounded with a further image D to form the final compound image.

Fig. 6 illustrates yet another embodiment in which the registration transforms undergone by each component frame are tracked and stored, and used to completely remove the component frame when the compounded image is updated with a current component

frame. At the top of the drawing the transform  $U$  necessary to register the estimates of frame  $A$  to those of frame  $B$  is computed and used to perform the registration of frame  $A$  to frame  $B$ , thus producing a two-frame compounded image  $B+A^U$ . Next, the transform  $V$  which registers the compounded image  $B+A^U$  to frame  $C$  is computed and used to perform the registration, thereby producing a three-frame compounded image  $C+B^V+A^{UV}$ . Note that frame  $A$  has now  
5 been processed by transforms  $U$  and  $V$ . In this example a three-frame compounded image is the desired result, which means that as the next frame  $D$  is registered and combined with the compounded image, the initial frame  $A$  is removed from the combination. This involves two process steps. In one of the process steps, the transform  $W$  which registers the compounded  
10 image  $C+B^V+A^{UV}$  to frame  $D$  is computed and used to perform the registration of the compounded image to frame  $D$ . In the other process step the transform  $UVW$ , representing the transforms previously experienced by frame  $A$ , are applied to frame  $A$  and subtracted from the compounded image. This removes all vestiges of frame  $A$  from the combination, since the transforms delineate the current locations of frame  $A$  data after all of the transformations  
15 undergone by the frame data. The frame  $A$  data is thus cleanly removed from the compounded image, leaving a new compounded image of the form  $D+C^W+B^{VW}$ . In the next step another new three-component compounded image,  $E+D^X+C^{WX}$  is produced which includes data from frames  $C$ ,  $D$ , and  $E$  after removal of frame  $B$  data by operation of the transform  $VWX$ , which tracks the changes experienced by previous registrations of frame  $B$ . It is seen that each  
20 subtraction cleanly removes the oldest component frame data by virtue of the use of the complete transform undergone by the oldest frame, and that a new compounded image for display is produced with the addition of each new component frame. This registration technique can advantageously be implemented with a single compound image accumulator, as more fully described in U.S. Pat. [appl. SN ATL-198] entitled "Ultrasonic diagnostic imaging  
25 system with real time spatial compounding processor".

The above embodiments of the present invention for conducting registration prior to compounding perform substantially equivalently as long as all the component frames have a high degree of similarity. In practice, however, the component frames do not always display the desired high degree of correlation due to "spatial artifacts" produced by non-  
30 uniform, anisotropic, or scattering properties of tissue such as:

1. highly attenuating tissues (e.g. fetal ribs, gall stones, certain types of tumors, etc.) can cause image artifacts called "acoustic shadows". These shadows are cast in a direction that depends on the angle of incidence of the ultrasound beam. A spatial compound image comprising component frames of different angles of incidence to the same target will

contain acoustic shadows in different locations, reducing the correlation between the component frames. The apparent decorrelation due to acoustic shadowing cannot be corrected by image registration methods, since registration of the shadows would cause misregistration of the real anatomy.

- 5 2. anisotropic reflectors such as tendons, bony surfaces, and the walls of blood vessels reflect ultrasound in a specular, mirror-like manner, producing artifacts called "highlight echoes." Highlight echoes shift position depending on the angle of insonification, creating decorrelation and/or apparent misregistration between component frames. Although it is generally desirable to acquire spatially diverse views of such specular targets so that they  
10 appear more continuous in the compound image, the resulting decorrelation and/or misregistration due to highlight artifacts can confound image registration methods and produce inaccurate registration results.
3. unresolved scatterers within tissue often produce a "texture pattern" superimposed on the ultrasound image. Although some of this pattern may be due to underlying regular or semi-  
15 regular microstructure, much of it is an undesirable, random mottling of the image known as "speckle." When the same tissue is imaged from independent spatial directions, the random speckle patterns are also independent, creating decorrelation from frame to frame that can contribute to inaccurate registration results.

In the presence of these spatial artifacts, the methods for registration prior to  
20 compounding do not all perform equivalently. For example, the reference frame method shown in Fig. 3 may fail to perform reliably if the component frames are acquired from substantially different directions. The resulting artifacts from shadowing or specular reflectors may prevent accurate registration prior to compounding. In this case, the pyramid method shown in Fig. 4 may perform better by registering spatially adjacent frames (with higher  
25 correlation) prior to compounding, followed by registration of the intermediate compound images. Fortunately, spatial compounding tends to improve the quality of the intermediate compound image by both filling-in specular reflectors more completely and reducing speckle. This potentially improves the quality of registration of the intermediate compound images prior to combining them into a final registered, compound image.

30 Another significant source of frame to frame decorrelation is due to motion of the scanhead in the direction perpendicular to the image plane (elevation motion decorrelation). When the clinical operator is searching for abnormalities (i.e. in a "survey mode") the probe is typically moved fairly rapidly in the elevation direction in order to view as much tissue as possible as quickly as possible. The result of elevation motion decorrelation

is that temporally sequential component frames become increasingly decorrelated as structures move out of the scan plan and their corresponding image features disappear. Again, the reference frame method shown in Fig. 3 may fail to perform reliably because elevation motion decorrelation over the entire acquisition sequence may prevent accurate registration prior to compounding. The pyramid method shown in Fig. 4 may perform better by registering temporally adjacent frames (with higher correlation) prior to compounding, followed by registration of the intermediate compound images.

A preferred technique for sensing misregistration, shown in Fig. 8, is to acquire a small number of "calibration" lines interspersed between each component frame. The ROI defined by these calibration lines is preferably viewed from a constant look direction and is used for misregistration sensing using SAD or other algorithms. As Fig. 8 shows, the calibration or reference lines acquired between component frames are used to compute SAD or otherwise to measure the degree of misregistration that has occurred during the time required to acquire a component frame. The calibration lines need not be at a regular line density or uniform angularity, but may be widely spaced and/or scattered across the image plane, and may be differently angled. A sparsely sampled frame will perform admirably. Although the additional lines will lower the overall frame rate, the temporal degradation need not be very great due to the low number of reference lines and, in any case, an adaptive approach can still give the user the sense of a satisfactorily high frame rate.

## CLAIMS:

1. An ultrasonic diagnostic imaging system, including an array transducer which is operated to acquire images at a plurality of different look directions, comprising:
  - a resampler which spatially registers component images of a compound image prior to compounding; and
  - 5 - a compound image processor, responsive to said resampler, which compounds images of different look directions to form a spatially compounded image.
2. The ultrasonic diagnostic imaging system of Claim 1, wherein said resampler comprises means for spatially registering a component image with a compound image of  
10 registered component images.
3. The ultrasonic diagnostic imaging system of Claim 2, wherein said compound image processor comprises means for combining a component image with a compound image with which said component image has been spatially registered.  
15
4. The ultrasonic diagnostic imaging system of Claim 1, wherein said resampler and said compound image processor comprise means for registering and compounding component images in the sequence in which they are acquired.
- 20 5. The ultrasonic diagnostic imaging system of Claim 1, wherein said resampler comprises means for registering component images which are not spatially adjacent.
6. The ultrasonic diagnostic imaging system of Claim 1, wherein said resampler comprises means for registering sequentially acquired component images; and wherein said  
25 compound image processor comprises means for compounding sequentially acquired and registered component images.

7. The ultrasonic diagnostic imaging system of Claim 1, wherein one of said component images comprises a reference image and wherein said resampler comprises means for registering other component images with said reference image.

- 5 8. The ultrasonic diagnostic imaging system of Claim 1, wherein said resampler and said compound image processor comprise:
- means for registering and combining component images to form intermediate compounded images; and
  - means for combining intermediate compounded images.

10

9. The ultrasonic diagnostic imaging system of Claim 8 wherein said resampler and said compound image processor further comprise:
- means for registering and combining intermediate compounded images.

- 15 10. The ultrasonic diagnostic imaging system of Claim 8, wherein said resampler and said compound image processor further comprise:
- means for registering and combining pairs of component images which are not temporally adjacent to form intermediate compounded images.

- 20 11. The ultrasonic diagnostic imaging system of Claim 1, wherein said resampler comprises a processor which calculates a metric representing the similarity or difference between component image frames.

- 25 12. The ultrasonic diagnostic imaging system of Claim 1, wherein said resampler comprises means for registering component images which are spatially adjacent.

13. The ultrasonic diagnostic imaging system of Claim 1, further comprising means for acquiring reference image data on a time interleaved basis with said component images; and
- 30 - wherein said resampler spatially registers component images on the basis of said reference image data.

14. The ultrasonic diagnostic imaging system of Claim 13, wherein said reference image data comprises groups of reference lines acquired between the times of acquisition of component images.
- 5 15. The ultrasonic diagnostic imaging system of Claim 14, wherein said reference lines exhibit a corresponding spatial alignment.

1/8

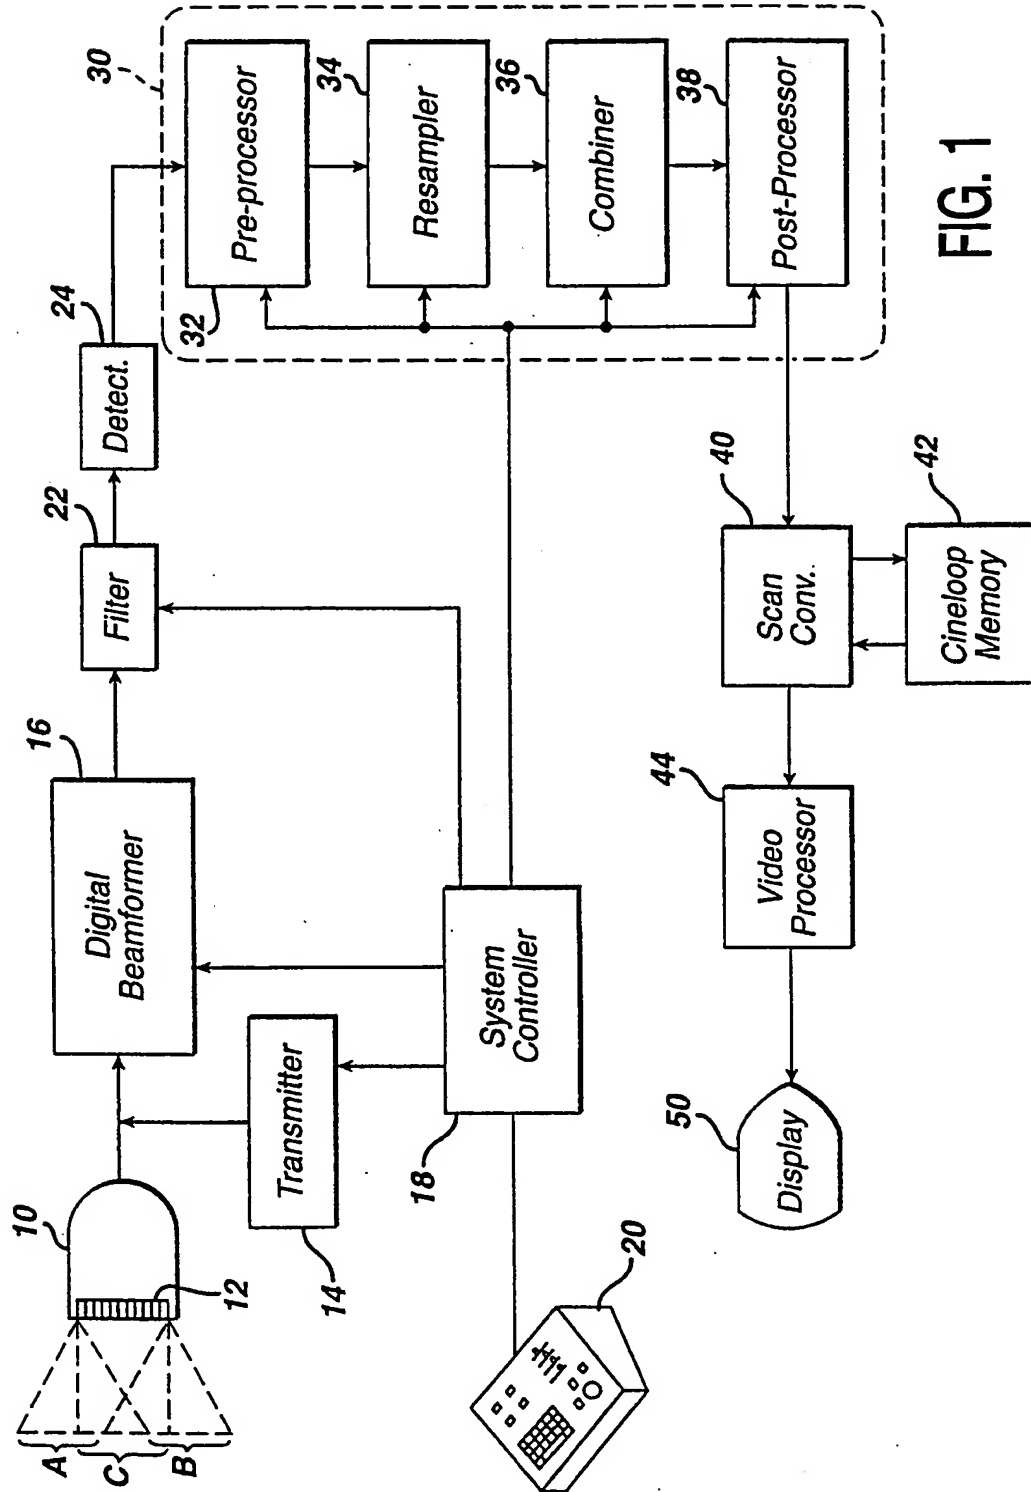


FIG. 1



2/8

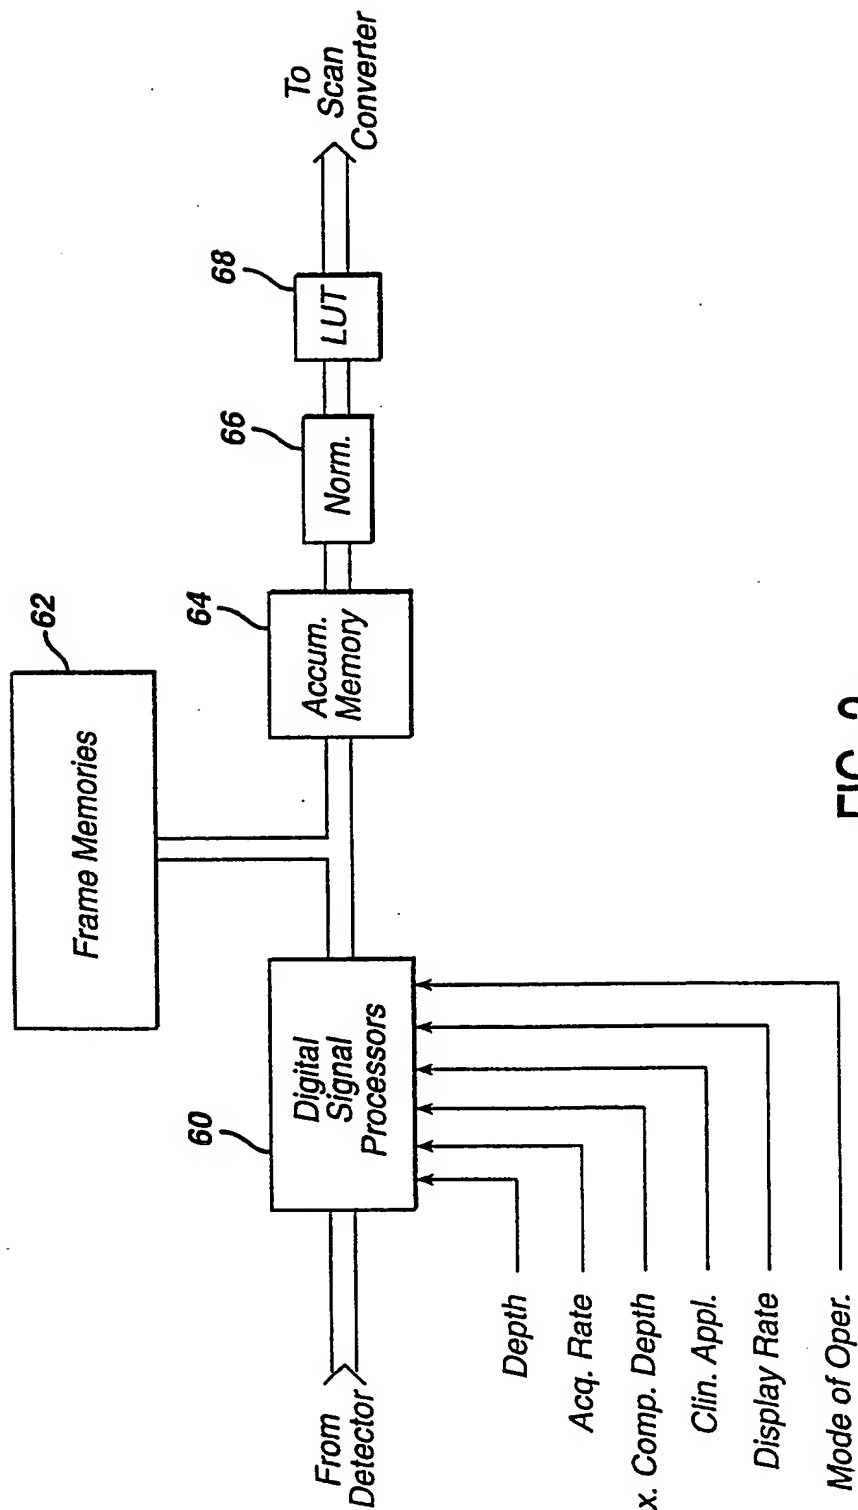


FIG. 2

3/8

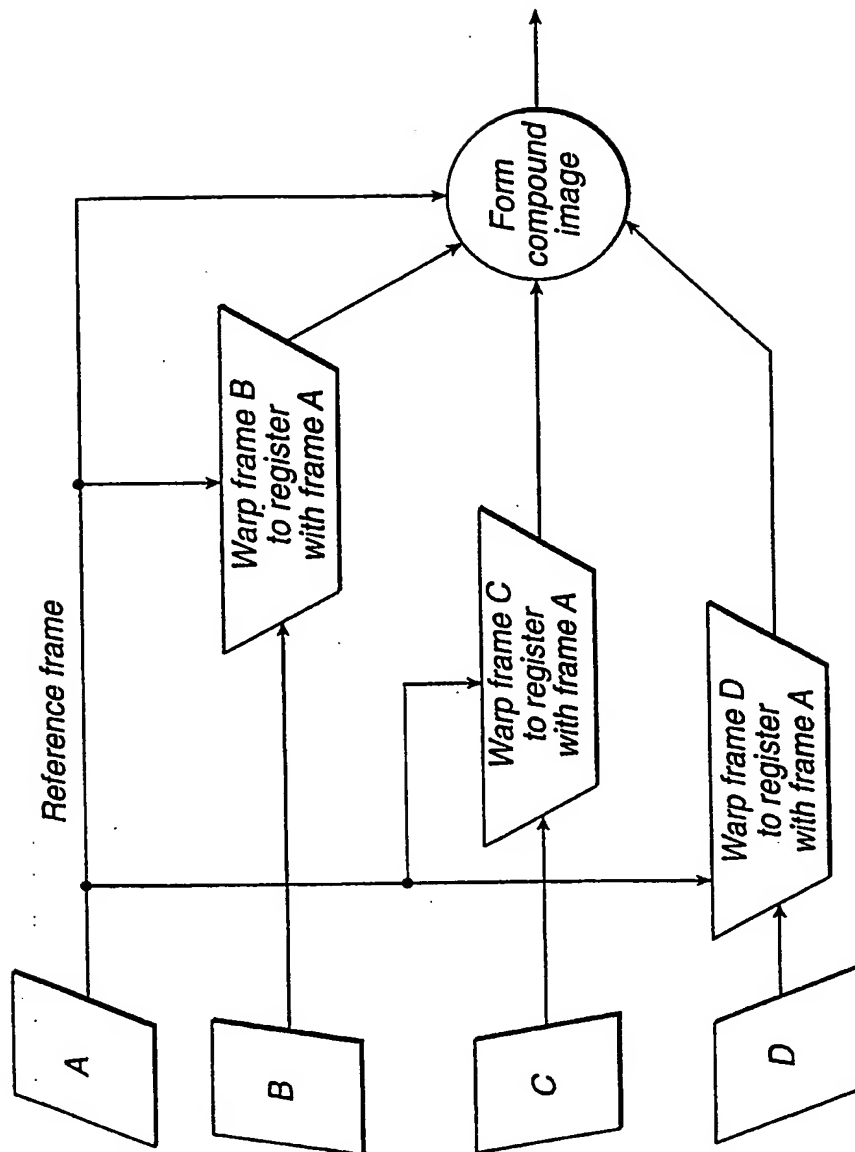


FIG. 3

4/8

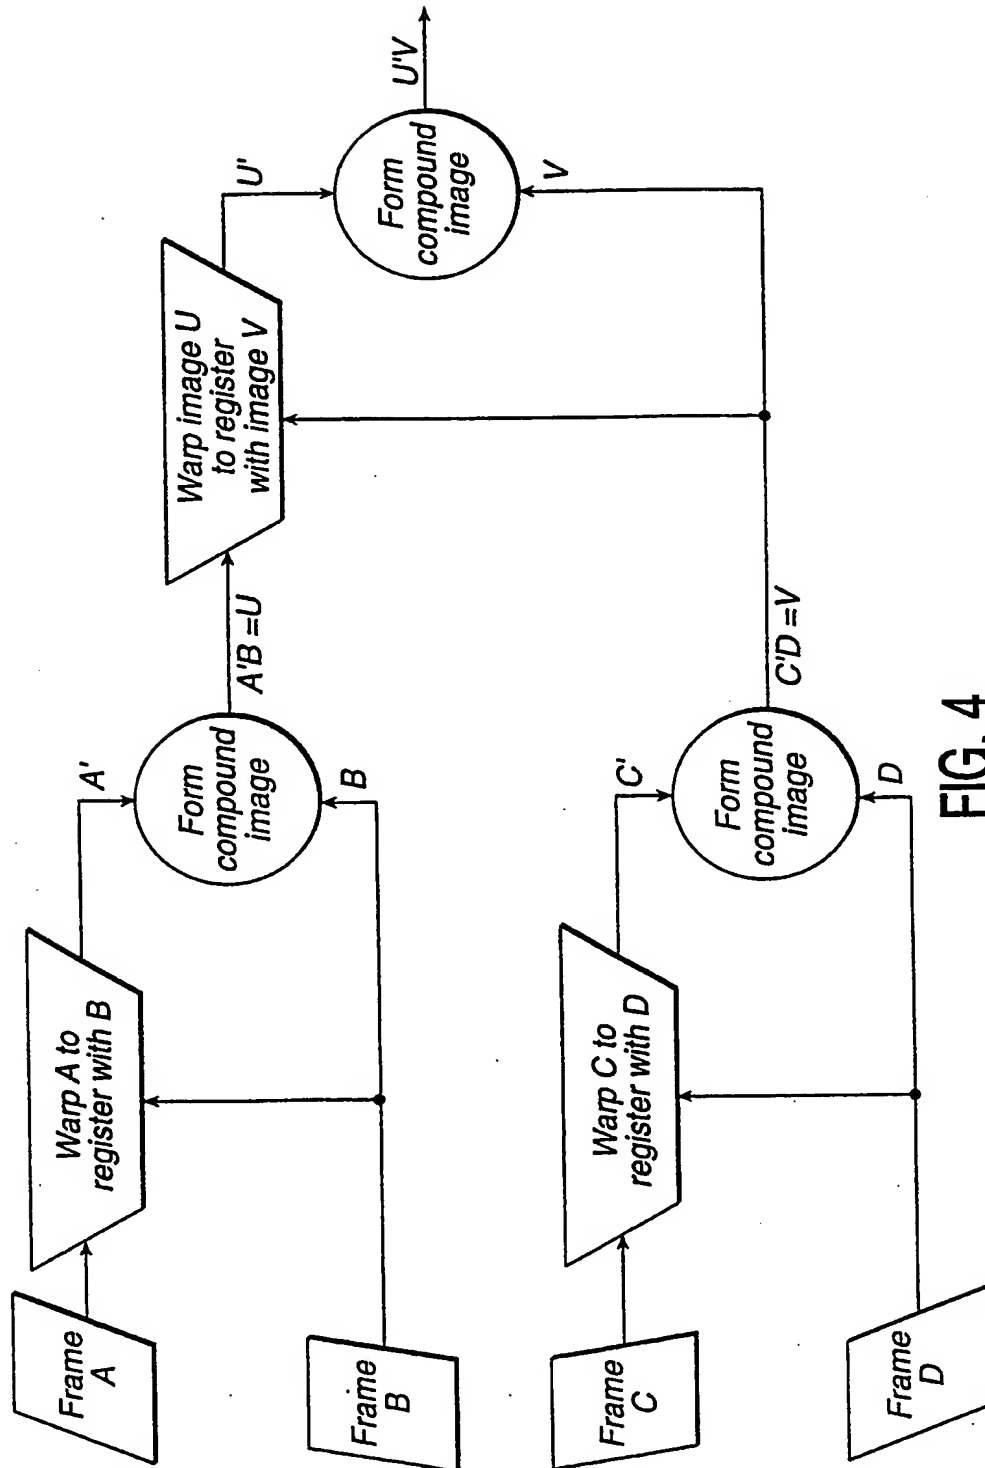


FIG. 4

5/8

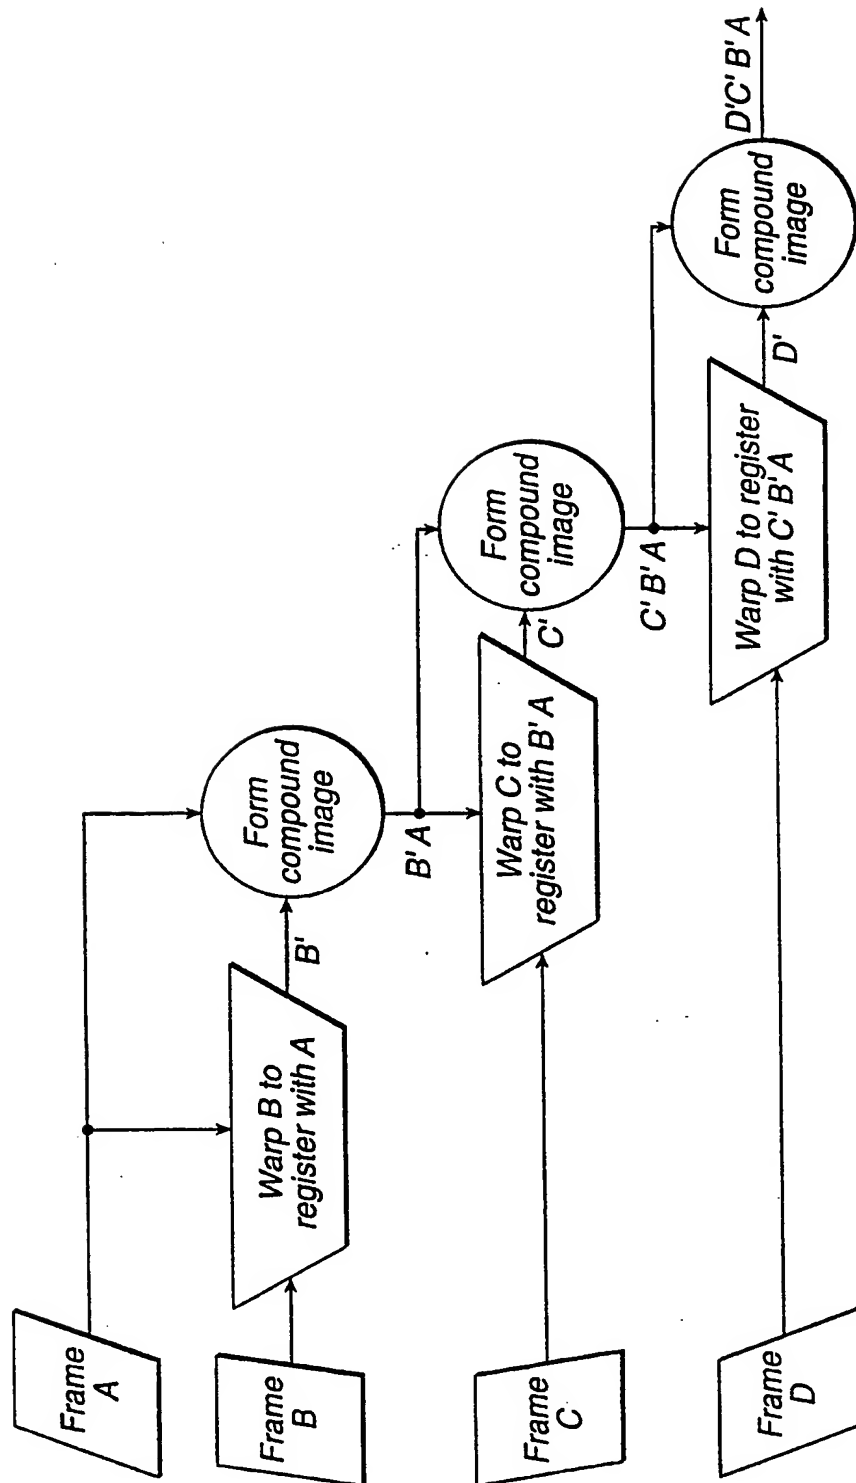


FIG. 5

6/8

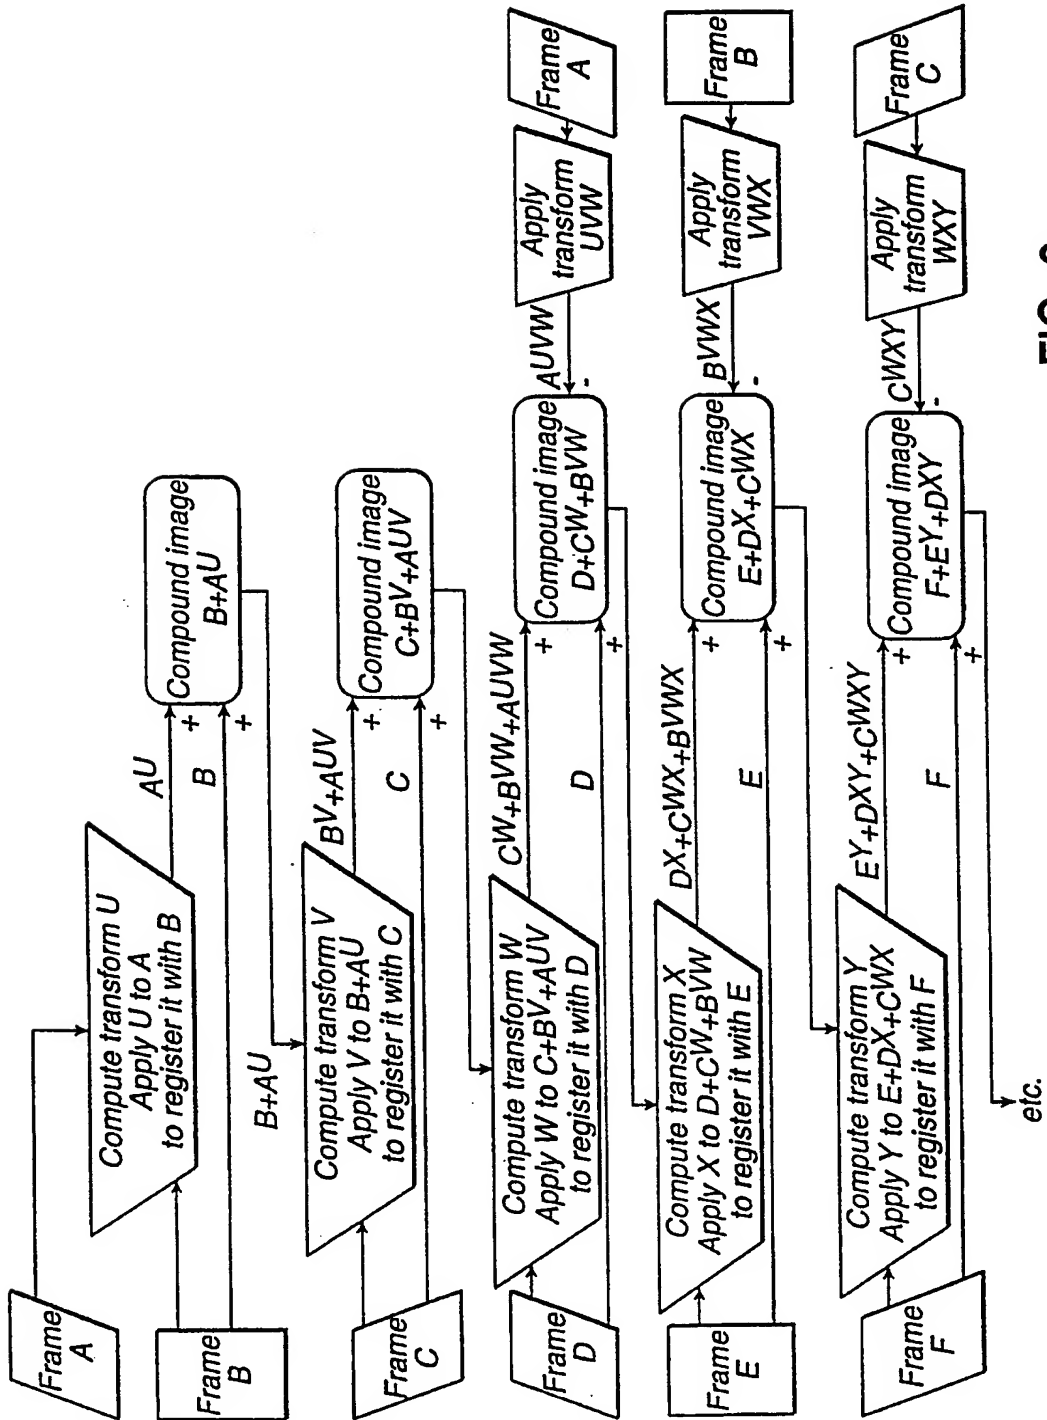


FIG. 6

7/8

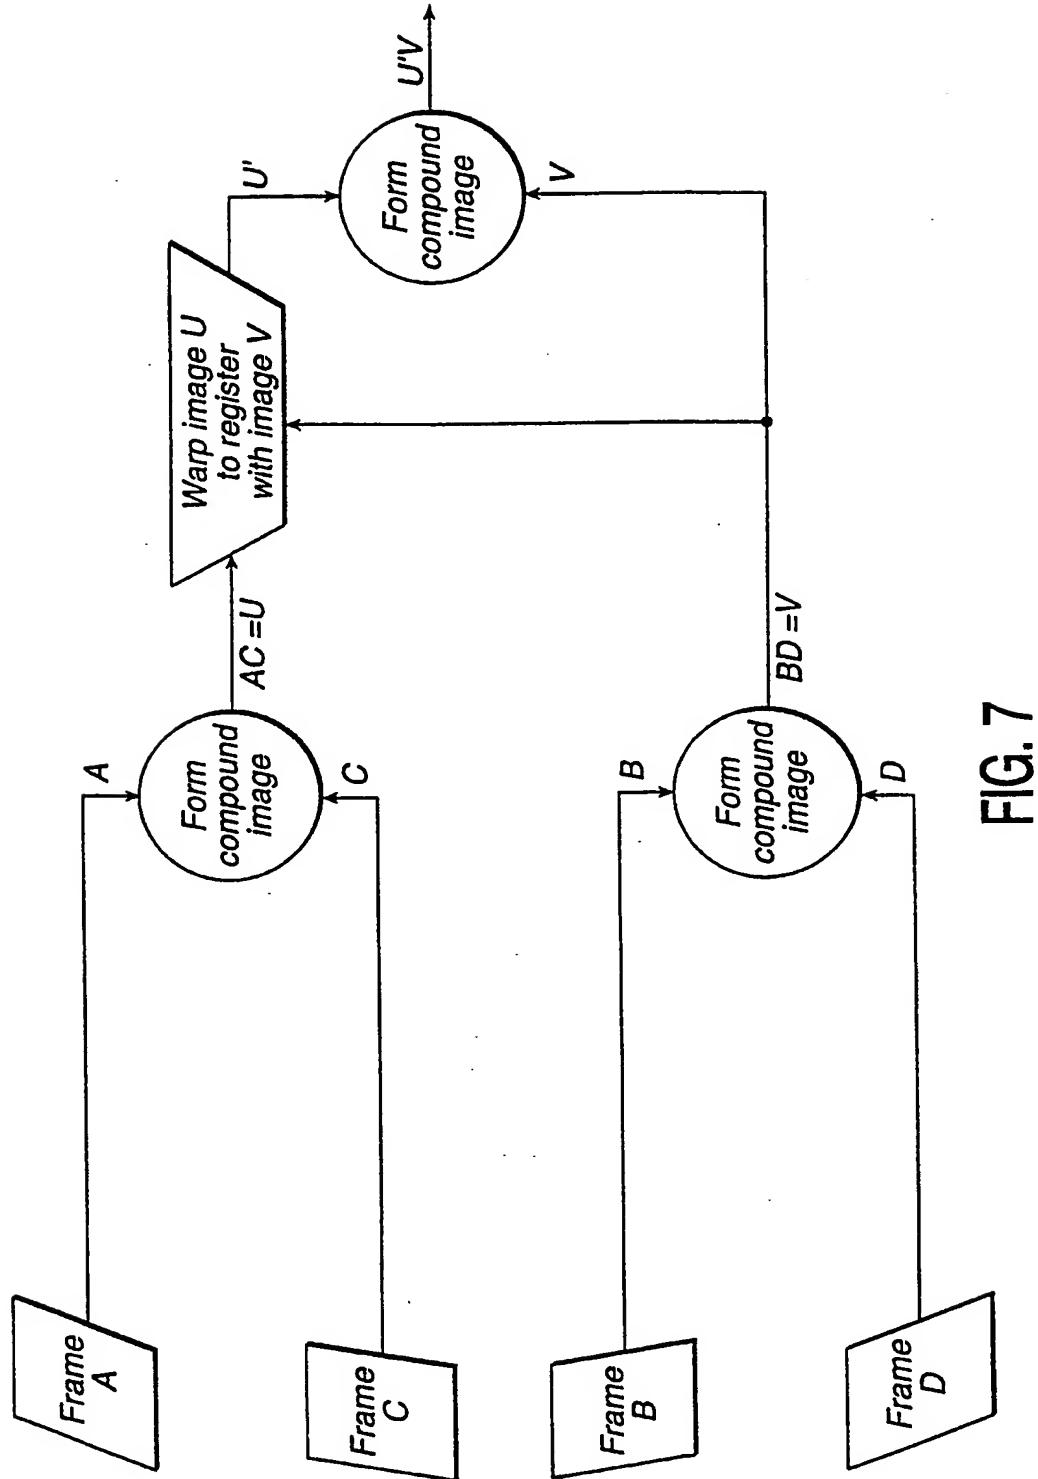


FIG. 7

8/8

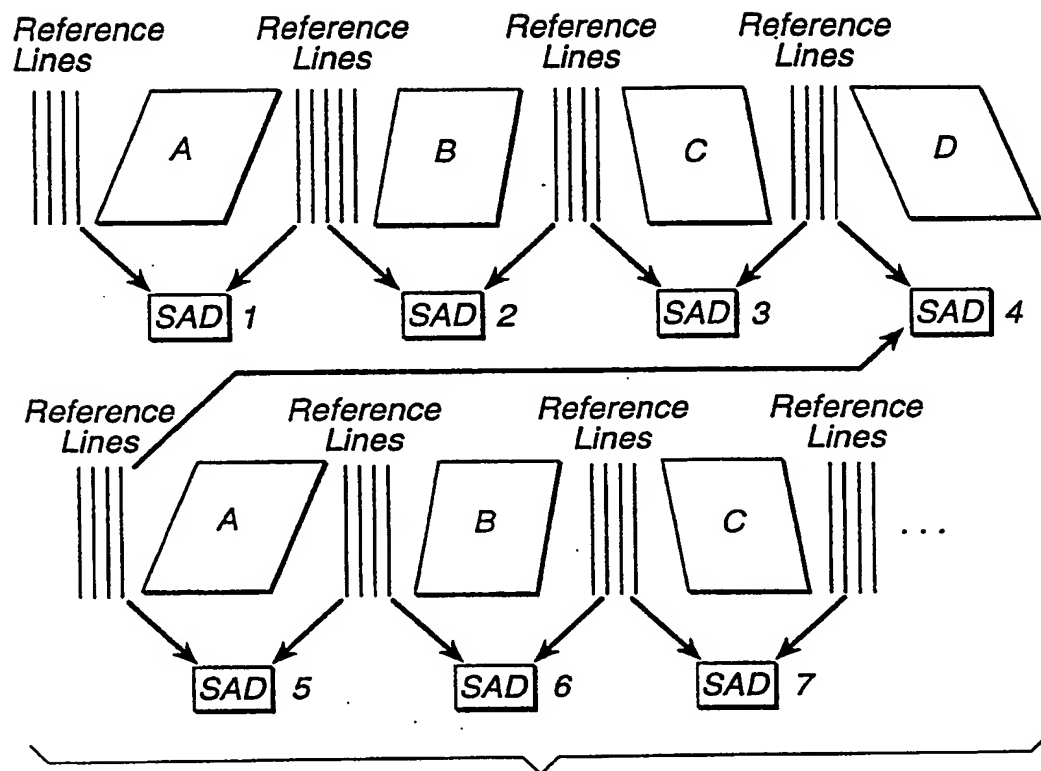


FIG. 8

# INTERNATIONAL SEARCH REPORT

International Application No.  
PCT/EP 99/07474

## A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 G01S7/52

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 G01S A61B G06T

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X A	DE 31 24 655 A (SIEMENS AG) 5 January 1983 (1983-01-05) page 10, line 16 -page 14, line 1; figures	1-4,8-11 5-7, 12-15
X	US 5 359 513 A (KANO AKIKO ET AL) 25 October 1994 (1994-10-25) column 4, line 56 -column 15, line 5; figures 1A-1D,11	1-4,6, 9-11
A	US 5 657 402 A (BENDER WALTER R ET AL) 12 August 1997 (1997-08-12) column 13 -column 20; figures 7,8	1-15
A	US 5 538 004 A (BAMBER JEFFREY C) 23 July 1996 (1996-07-23) column 11 -column 15; figures	1-7, 13-15
	-/--	

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

### \* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"Z" document member of the same patent family

Date of the actual completion of the international search

10 January 2000

Date of mailing of the international search report

14/01/2000

Name and mailing address of the ISA  
European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax: (+31-70) 340-3016

Authorized officer

Devine, J



# INTERNATIONAL SEARCH REPORT

International Application No

PCT/EP 99/07474

## C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 5 779 641 A (HATFIELD WILLIAM THOMAS ET AL) 14 July 1998 (1998-07-14) abstract; claims; figures ---	1-15
A	ELAD M ET AL: "RESTORATION OF A SINGLE SUPERRESOLUTION IMAGE FROM SEVERAL BLURRED, NOISY, AND UNDERSAMPLED MEASURED IMAGES" IEEE TRANSACTIONS ON IMAGE PROCESSING, US, IEEE INC. NEW YORK, vol. 6, no. 12, page 1646-1658 XP000724632 ISSN: 1057-7149 ---	1-15
A	MOSKALIK A ET AL: "REGISTRATION OF THREE-DIMENSIONAL COMPOUND ULTRASOUND SCANS OF THE BREAST FOR REFRACTION AND MOTION CORRECTION" ULTRASOUND IN MEDICINE AND BIOLOGY, US, NEW YORK, NY, vol. 21, no. 6, page 769-778 XP002060900 ISSN: 0301-5629 page 772 -page 773 -----	1-15

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/EP 99/07474

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
DE 3124655	A	05-01-1983	JP 58005649 A	13-01-1983
US 5359513	A	25-10-1994	JP 7037074 A	07-02-1995
US 5657402	A	12-08-1997	JP 8503088 T	02-04-1996
			WO 9410653 A	11-05-1994
			US 5920657 A	06-07-1999
			JP 5304675 A	16-11-1993
US 5538004	A	23-07-1996	NONE	
US 5779641	A	14-07-1998	DE 19819831 A	19-11-1998
			JP 11028211 A	02-02-1999

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

**BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☒ FADED TEXT OR DRAWING
- ☒ BLURRED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☐ COLOR OR BLACK AND WHITE PHOTOGRAPHS
- ☐ GRAY SCALE DOCUMENTS
- ☐ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☒ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☐ OTHER: \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**